

#### **FORM #HLIT 205-2G**

TEL 1-800-696-6165 www.comoso.com

#### I. INTRODUCTION

The Flow Meter is a rugged industrial class in-line flow rate indicator, offered in aluminum, brass or stainless steel models to monitor a wide variety of liquids. Available in seven port sizes from ¼" to 3" for flow ranges from .02-0.2 (0.1-0.75) through 20-300 GPM (100-1100 LPM), meters are calibrated at 0.876 specific gravity for oil or other petroleum-based fluids, 1.0 for water or other water-based fluids, or 1.18 for phosphate ester liquids.

The flow meter is equipped with a 360° rotatable guard/scale which allows the meter to be installed in any orientation without regard to scale direction. Once the meter is permanently installed, the guard/scale can be rotated 360° to optimize readability.

In addition, the unique spring loaded design of this variable area flow meter decreases viscosity sensitivity and allows it to be installed in any position, including inverted, without affecting accuracy. An optional inverted scale is available for these applications.

The standard flow meter is a unidirectional device. If required, a reverse flow by-pass option is available for the oil, phosphate ester and water-based fluid models. Note that flow is measured in the forward direction only.

**Aluminum** models are offered as a rugged, low cost flow meter for monitoring noncorrosive water-based or petroleum-based fluids under operating pressures up to 3500 psi (241 bar).

**Brass** meters are recommended for water monitoring applications or other systems where corrosion inhibitors are not present.

**Stainless Steel** is available for monitoring hydraulic systems operating at pressures up to 6000 psi (414 bar) or other corrosive caustic fluids, such as acetic acid. For further construction material information, see "Fluid Selection Chart" in the Appendix.








#### II. OPERATING PRINCIPLE

The Flow Meter is a variable area instrument. A sharp-edged Orifice①, located within the Piston Assembly②, forms an annular opening with the contoured Metering Cone③. The piston assembly carries a cylindrical PPS/Ceramic Magnet④ that is magnetically coupled to an external Indicating Magnet which moves precisely in direct response to movement of the piston. A calibrated Spring⑥ opposes flow in the forward direction.

The Hedland variable area flow meters are the most readable products in their class. Brightly colored indicators move over the graduated, linear Flow Scale which contains bold, easy to read numeral and gauge marks. The enhanced resolution virtually eliminates parallax problems associated with competitive, direct reading flow meters.

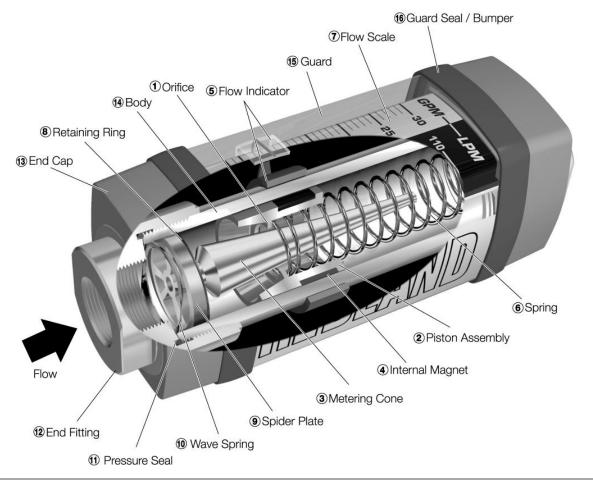

Page 2 Form #HLIT 205-2G 11/10



#### III. SPECIFICATIONS

#### **Temperature Range**

- Standard: -20 to +240 °F (-29 to +116 °C)
- High Temp & Hostile Environment:
   -20 to +400 °F (-29 to +205 °C) Continuous;
   +400 to +500 °F (+205 to +260 °C) Intermittent
- See Appendix for Pressure vs. Temperature correlation information

#### Pressure Rating (3:1 safety factor)

- Aluminum/Brass Models: 3500 psi (241 bar) maximum
- Stainless Steel Models:
   ½" & ½" Sizes; 6000 psi (414 bar) maximum
   ¾"thru 1-½" Sizes; 5000 psi (345 bar) maximum

#### **Pressure Drop**

• See Appendix for specific meter information

#### **Accuracy**

• ±2% of full scale

#### Repeatability

• ±1%

#### Threads

 SAE J1926/1, NPTF ANSI B2.2, BSPP ISO1179, Code 61 and Code 62: SAEJ518

#### Test Kit Pressure Gauge - Glycerin Dampened

- Aluminum/Brass Models: 0-3,500 psi (0-240 bar)
- Stainless Steel Models: 0-6,000 psi (0-400 bar)

#### **Test Kit Load Valve**

- 1/2", 3/4" and 1" Sizes: Needle valve
- 1-1/4" and 1-1/2" Sizes: Ball valve
- Produce ΔP up to 3,500 psi (241 bar) PSID and 6,000 psi (414 bar) PSID

#### **Dimensions**

See Appendix

#### Materials of Construction - Basic Flow Meters and Test Kits

Meter Model	Body	Piston	Cone	Spider Plate	Spring	Fasteners	Pressure Seals	Guard	Retaining Ring	Retaining Spring	Indicator & Internal Magnet	Guard Seal/Bumper	Scale Support	End Caps
Oil		"351 Anodized Alumininum C360 Brass 1		T04000	T00000	T00000	Viton <sup>®</sup>	Deberation	SAE 1070/1090	SAE 1070/1090	BB0/0	Down N	6063-T6	No.
Basic & Test Kit	T303SS	2024-T351 Anodized Alumininum		T316SS	T302SS	T303SS	viton-	Polycarbonate	Carbon Steel	Carbon Steel	PPS/Ceramic	Buna N	Aluminum	Nylon ST
	2024-T35	1 Anodized Al	lumininum											
PE Basic &	C360 Brass		T316SS	T302SS	T303SS	EPR	Polycarbonate	SAE 1070/1090	SAE 1070/1090	PPS/Ceramic	EPR	6063-T6	Nylon ST	
Test Kit	T303SS	2024- Anodized A		131000	100200	130300	Erik		Carbon Steel	Carbon Steel			Aluminum	,.51101
	2024-T35	1 Anodized A	Anodized Alumininum											
WBF Basic &		C360 Brass 1		T316SS	T00000	T303SS	Viton®	Debessehenste	T04000	T04000	DD0/0	Down N.	6063-T6	Notes OT
Test Kit	T303SS	2024- Anodized A		131655	T302SS	130355	viton-	Polycarbonate	T316SS	T316SS	PPS/Ceramic	Buna N	Aluminum	Nylon ST
Water							0						6063-T6	
Basic Only	T303SS	C360 Brass		T316SS	T302SS	T303SS	Viton®	Polycarbonate	T316SS	T316SS	PPS/Ceramic	Buna N	Aluminum	Nylon ST

#### Materials of Construction - A.P.I. Oil / Caustic and Corrosive Liquids

Meter Model	Body	Piston	Cone	Spider Plate	Spring	Fasteners	Pressure Seals	Guard	Retaining Ring	Retaining Spring	Indicator & Internal Magnet	Guard Seal/Bumper	Scale Support	End Caps
Standard		T316SS		T316SS	T316SS	T316SS	Viton <sup>®</sup>	Polycarbonate	T316SS	T316SS	PPS/Ceramic	Buna N	6063-T6 Aluminum	Nylon ST
Meter Model				Spider			Pressure		Retaining	Retaining				
Weter Woder	Body	Piston	Cone	Plate	Spring	Fasteners	Seals	Guard	Ring	Spring		Bumper	Scale Support	End Caps



#### **Materials of Construction - High Temp Flow Meters**

Meter Model	Body	Piston	Cone	Spider Plate	Spring	Fasteners	Pressure Seals	Guard	Retaining Ring	Retaining Spring	Indicator / Internal Magnet	Bumper	Scale / Scale Support	End Caps
Oil	2024-T35	T351 Anodized Alumininum C360 Brass		T316SS	T302SS	T303SS	Viton <sup>®</sup>	Cylindrical	SAE 1070/1090	SAE 1070/1090	Indicator: Nickel-plated Carbon Steel	2011-T3 Anodized	Scale: Polymide Scale Support:	2011-T3 Anodized
	T303SS	2024 Anodized A	-T351 Alumininum	101000	100200	100000	***************************************	Pyrex <sup>®</sup> Glass	Carbon Steel	Carbon Steel	Magnet: Teflon® Coated Alnico 8	Aluminum	T316SS	Aluminum
PE	2024-T351 A		lumininum	T316SS	T302SS	T303SS	FPR	Cylindrical	SAE 1070/1090	SAE 1070/1090	Indicator: Nickel-plated Carbon Steel	FPR	Scale: Polymide Scale Support:	2011-T3 Anodized
F	T303SS	2024 Anodized A	-T351 Alumininum	131033	130233	130333		Pyrex <sup>®</sup> Glass	Carbon Steel	Carbon Steel	Magnet: Teflon® Coated Alnico 8			Aluminum
	2024-T35	1 Anodized A	lumininum		T302SS		Viton <sup>®</sup>	Cylindrical Pyrex <sup>®</sup> Glass	T316SS	T316SS	Indicator: Nickel-plated	Buna N	Scale: Polymide Scale Support:	2011-T3 Anodized
WBF .		C360 Brass 1		T316SS		T303SS					Carbon Steel			
	T303SS		-T351 Alumininum					Pyrex Glass			Magnet: Teflon® Coated Alnico 8		T316SS	Aluminum
Water			C360 Brass		T00000	T00000	Viton <sup>®</sup>	Cylindrical	T316SS	T316SS	Indicator: Nickel-plated Carbon Steel	Buna N	Scale: Polymide	2011-T3
vvater	T303SS	C360	C360 Brass		T302SS	T303SS	viton"	Pyrex <sup>®</sup> Glass	131855		Magnet: Teflon® Coated Alnico 8		Scale Support: T316SS	Anodized Aluminum
1 3" Mode	ls have Celco	n® piston/pis	ton ring											

#### IV. INSTALLATION

### **A** CAUTION

This product should be installed and serviced by technically qualified personnel trained in maintaining industrial class flow instrumentation and processing equipment.

### **A** CAUTION

Read instructions thoroughly before installing the unit. If you have any questions regarding product installation or maintenance, call your local supplier for more information.

### A CAUTION

Oil meters are not recommended for water monitoring applications. If meter is to be subjected to both oil and water, water meters (brass) are suggested. Consult factory for details.

### **A** CAUTION

This meter may contain residual amounts of test fluid at the time of shipment. This fluid should be removed prior to installation as the fluid may be incompatible or hazardous with some liquids or gases. Failure to follow these instructions could result in damage to the equipment.

### **A** CAUTION

This standard meter is unidirectional. Attempts to flow fluids in the opposite direction of the flow arrow will result in the meter acting as a check valve, creating a deadheading situation. If the differential pressure magnitude is great enough, damage to the internal parts of the meter will result.

Page 4 Form #HLIT 205-2G 11/10



#### Installation Recommendations

The in-line flow meter is a simple device to install. However, the following measures are recommended for reliable, trouble-free operation:

**Do -** Align pipe accurately. Piping should be accurately aligned and of correct length. The high pressure body of the flow meter can withstand shock and flow/pressure pulsation. However, the piping should be firmly supported by external mounting brackets, both upstream and downstream of the meter, to avoid any pipe flexing actions that could reduce meter life.

**Do -** Use rigid mounting. If the flow meter inlet or outlet are to be rigidly mounted, and the opposing port is to be connected to flexible hose, the end connected with the flexible hose must be rigidly mounted.

Do - Use Teflon® tape for sealing NPT fitting.

**Do -** Install unions. Install a union near the inlet or outlet of the meter. This will facilitate quick, easy meter removal and inspection during periodic maintenance procedures.

**Do -** Mount the meter either horizontally or vertically (flow arrow pointing to either side or straight up). If the meter must be mounted inverted, special inverted scales are available from the factory.

**Do -** Ensure the fluid is traveling in the direction of the flow arrow (**Figure 3** on page 6).

**Do -** Use at least a 200 mesh (74 micron) filter. The meter will allow particulate to pass that would jam most valves and flow controls. Systems that do not have filtration should be equipped with at least a 200 mesh (74 micron)

filter. Most hydraulic systems already have much finer filtration.

Dirt, ferrous metal or sealing agents, such as Teflon® tape may lodge and cause malfunction. If the meter is jammed at a fixed position, follow cleaning and maintenance instructions.

**Don't -** Use thread locking compounds as thread sealant.

**Don't -** Install the flow meter near turbulence producing fittings such as elbows, reducers, close coupled valves, etc. The in-line flow meter does not require flow straighteners or special lengths of straight inlet/outlet piping to stabilize turbulent flow patterns. However, to assure maximum operational reliability, avoid installation of elbows, valves and/or reducers immediately adjacent to the meter inlet.

**Don't -** Install the meter near fast-acting valves. Fast-acting valves have the potential to create high magnitude hydraulic pressure spikes. These spikes can damage the internal components of the meter, resulting in inaccuracies or malfunction.

**Don't** - Allow unidirectional meters to be operated against the direction of the flow arrow. The standard flow meter is an unidirectional flow meter. The piston acts as a check valve to block flow in the reverse direction. This causes an excessive pressure differential, which can result in damage to internal meter components. The flow meter is also available in a modified design, which offers a reverse flow by-pass feature to accommodate bi-directional flow.

NOTE: In-line meters with a reverse flow bypass feature are available. Consult factory for details.



#### **Installing the Flow Meter**

- 1. Mount the meter so fluid is traveling in the direction of the flow arrow. See **Figure 3**.
- Select a mounting location that is suitable for viewing and product service. To connect the flow meter into the piping system, place an open-ended wrench onto the flow meter wrench flats adjacent to the pipe connection being installed. DO NOT wrench on the opposite end of the flow meter or leakage may result. See Figure 4.
- 3. After installation, rotate meter by hand to view flow scale. See **Figure 5**.

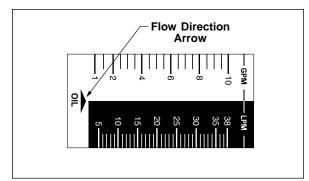


Figure 3. Flow Direction Arrow

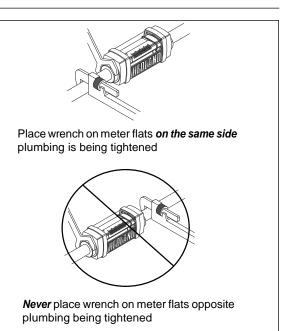


Figure 4. Installing Meter

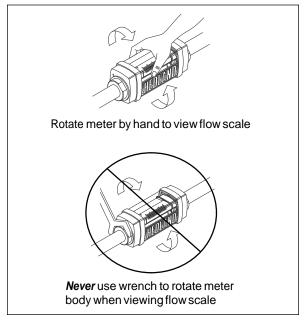


Figure 5. Rotating Meter

Page 6 Form #HLIT 205-2G 11/10



#### **Installing the Test Kit Flow Meter**

- Mount the VA High Pressure Test Kit Flow Meter so fluid is traveling in the direction of the flow arrow. See Figure 3 on page 6.
- 2. Install the test kit at any location in the hydraulic circuit that is suitable for viewing. To connect the test kit into the piping system, place an open-ended wrench onto the test kit valve on the inlet side or on the test kit wrench flat on the outlet side adjacent to the pipe connection being installed. DO NOT wrench on the opposite end of the test kit or leakage may result. See Figure 6.

Or, use quick disconnect couplings for easy connections and to keep the test kit sealed and clean when not in use. Diagrams illustrating Typical Test Placements for the test kits are located in the Test Procedures section beginning on page 8.

3. After installation, rotate meter by hand to view flow scale. See **Figure 7**.

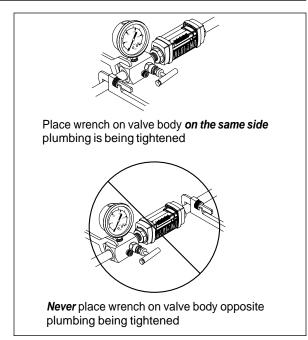


Figure 6. Installing Test Kit




Figure 7. Rotating Test Kit



#### IV. OPERATION

#### **General Information**

NOTE: Refer to the Appendix for application information and fluid charts.

#### **Test Kit Information**

# ALWAYS START WITH THE LOADING VALVE OPEN



All Test Kits are shipped with the loading valve in the closed position. The loading valve must be opened fully before initiating flow and testing of the hydraulic circuit. Turn the loading valve handle counterclockwise to the fully open position. Failure to open the loading valve fully can result in injury to personnel and/or damage to the equipment.

#### V. TEST PROCEDURES FOR TEST KIT FLOW METERS



The information in this manual is for general application only. Any information furnished by the manufacturer of the machine's hydraulic components should be followed. Specific systems may require specific test procedures.

#### **General Information**

The VA High Pressure Test Kits are designed to measure flow and pressure. Power measurements are derived from the product of flow and pressure. When using a Test Kit, power can be calculated using the following formulas:

H.P. = 
$$\frac{\text{GPM} \times \text{PSI}}{1714}$$
 H.P. =  $\frac{\text{liters/min} \times \text{bal}}{447.4}$   

$$\text{kW} = \frac{\text{liters/min} \times \text{bar}}{600}$$

#### **Standard Test Conditions**

- 1. Install the Test Kit as described in one of the following test procedures:
  - a. Pump Test
  - b. "Tee"Test
  - c. Relief Valves in Separate Housings
  - d. Relief Valves
- 2. Open the loading valve fully by turning the handle counterclockwise.
- 3. Start the pump and adjust it to rated speed.
- 4. Open the Test Kit loading valve fully and proceed with the required test procedure.
- 5. The Test Kit will indicate flow and pressure.

#### Pump Test (See Figure 8 on page 9)

A tee must be installed between the pump discharge port and the return line to the tank. Be sure the fluid path is only through the pump, the hydraulic test unit, and back to the tank.

- 1. Plug the line to the control valve.
- 2. Open the Test Kit loading valve fully to read maximum pump flow at zero pressure.

Page 8 Form #HLIT 205-2G 11/10






Figure 8. Pump Test

- Close the loading valve to increase pressure from zero pressure to rated or maximum pump pressure to determine pump condition.
- 4. The pump flow at rated pressure can now be checked against the pump manufacturer's specifications. A decrease in flow from zero pressure to maximum pressure indicates the pump condition. A pump that delivers a constant low flow at zero pressure and at maximum pressure suggests suction problems.

#### "Tee" Test (See Figure 9)

A tee must be installed between the pump and control valve and connected to the inlet of the Test Kit. The outlet port of the Test Kit is connected to the tank. Pumps and relief valves can be isolated from the system and checked with the "Tee" Test.

- 1. Pump Test
  - a. Plug the line to the control valve.

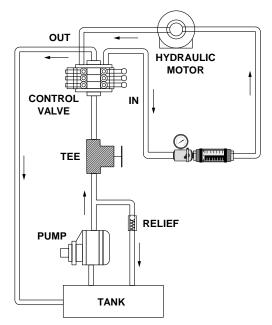


Figure 9. "Tee" Test

- Open the Test Kit loading valve fully to read maximum pump flow at zero pressure.
- c. Close the loading valve to increase pressure from zero pressure to rated or maximum pump pressure to determine pump condition.
- d. The pump flow at rated pressure can now be checked against the pump manufacturer's specifications. A decrease in flow from zero pressure to maximum pressure indicates the pump condition. A pump that delivers a constant low flow at zero pressure and at maximum pressure suggests suction problems.



#### 2. Relief Valve Test

- a. Put a control valve into a power output mode with the output flow blocked, such as a cylinder at the end of its stroke.
- b. Close the Test Kit loading valve while viewing the pressure. Pressure will increase until the relief valve opens. Record the pressure at this point. Repeat to check the relief valve adjustment.

#### **Relief Valve in Separate Housing**

- Install the Test Kit in a "Tee" Test configuration to the line connecting the pump and relief valve. Plug any extra outlets.
- 2. Close the Test Kit loading valve and watch the pressure and flow.
  - a. Reconnect the control valve to the tee. Put a control valve into a power output mode with the output flow blocked, such as a cylinder at the end of its stroke.
  - b. Close the Test Kit loading valve while watching the pressure. Pressure will increase until the relief valve opens. Record the pressure at this point. Repeat to check the relief valve adjustment.

#### **Relief Valves**

Often relief valves will start to open before they reach their full pressure flow settings. This can be noted by comparing the pressure and flow rate readings made in Step 3 under "Tee" Test. Any great decrease in flow rate from tests made in Step 3 under "Tee" Test indicates a faulty relief valve.

#### VI. MAINTENANCE



#### **WARNING**

Before attempting to remove the flow meter from the line, check the system to confirm that line pressure has been reduced to zero PSI. Failure to follow these instructions could result in serious personal injury or death and/ or damage to the equipment.

1. Remove the flow meter from the line. Remove excess piping from meter.

NOTE: It is not necessary to remove the transparent dust guard from the meter to remove the meter from the line. If you choose to remove the dust guard assembly, refer to Removal of Dust Guard section on page 11.

Thoroughly wipe off the entire flow meter surface using mild detergent or isopropyl alcohol.



### **CAUTION**

Do not use aromatic hydrocarbons, halogenated hydrocarbons, ketones or ester based fluids on polycarbonate lens. Failure to follow these instructions could result in damage to the meter.

Page 10 Form #HLIT 205-2G 11/10



- 3. Remove the inlet cap from the flow meter, noting the sequence of disassembly for later reference (during reassembly).
- 4. The internal parts are secured with a retaining ring. Remove the retaining ring and the internal wetted parts from the flow meter.

NOTE: If internal parts do not slide freely from flow meter, use a wooden dowel inserted into the outlet port of the meter to push parts out.

 Place all parts on a clean work surface.
 Clean and inspect all parts. Replace any that appear worn or damaged.

Check inlet port O-ring for damage and replace if required.



### **CAUTION**

Field replacement of the spring, metering cone and/or piston/magnet assembly may result in changes to the calibration of the flow meter.

- Reassemble spring, then piston/magnet assembly and retaining ring into flow meter.
- Install metering cone/spider plate assembly, retaining spring, and secure with inlet cap.
- 8. Reinstall meter to the line.

#### **Removal of Dust Guard**

To remove the dust guard for cleaning or replacement, simply loosen the end fitting located at the bottom of the meter and slide the end cap, dust bumper, and the dust guard off the bottom of the meter, taking care to avoid damaging the O-ring seal between the end cap and the dust gland.

#### **Quick Re-Coupling**

This piston-type variable area flow meter is inherently less sensitive to shock and vibration than other variable area designs. The unique magnetic coupling also eliminates the need for mechanical linkages that can wear or loosen over the functional life of the meter.

However, on occasion, a pressure spike or extreme flow surge can cause the piston to move at such rapid speed that it disconnects the piston magnet and the external indicator ring. If this occurs, use one of these procedures to recouple the magnet and the external indicator ring:

- If the system permits, simply change flow rate from "no flow" to "full flow" allowing the moving piston to magnetically recouple to the indicator ring.
- For rigorous cyclical applications where de-coupling may occur frequently, consult the technical services staff for further recommendations.

#### **Test Kit Maintenance**

#### Load Valve

If the valve fails to load the system, remove the valve body and check for foreign material, worn parts or seals.

#### Flow

The absence of any flow reading may indicate a seized piston assembly. Remove any material that may be preventing the piston to slide.

If the Test Kit still fails to indicate flow, it is recommended to return the Test Kit to the factory. For return procedures, see the Return Goods Authorization section of this manual on page 19.



#### VII. APPENDIX

#### **Application Information**

#### Viscosity Effect (SUS/cSt)

The design utilizes a precision machined, sharpedged orifice and biasing calibration spring that assures operating stability and accuracy over the wide viscosity range common to many fluids. Generally, high flow models of each meter size provide good accuracy over a viscosity range of 40 to 500 SUS (4.2 to 109 cSt).

#### Density Effect (specific gravity)

Any fluid density change from stated standards has a proportional effect on meter accuracy. Special scales can be supplied if actual specific gravity decreases accuracy beyond application limits. Corrections for more or less dense fluids can be made to standard scales using the following correction factors:


for water/water-based meters

for petroleum-based meters

#### Fluid Selection Chart

			on Factor ard Scale	Int	terna Mate		dy	Pres	rnal sure als		Dust Suar	
Fluid	Specific Gravity	Oil	Water	Aluminum	Brass	T316SS	T303SS	Viton	EPR	Polycarbonate	Nylon	Pyrex
Acetic Acid (Air-Free)	1.06	0.909	0.971	С	N	R	R	R	R	С	N	R
Acetone	0.79	1.053	1.125	R	R	R	R	N	R	N	R	R
Alcohol Butyl (Butanol)	0.83	1.027	1.098	С	С	R	R	С	R	R	R	R
Alcohol Ethyl (Ethanol)	0.83	1.027	1.098	С	С	R	R	С	R	R	N	R
Ammonia	0.89	0.992	1.060	R	С	R	R	N	R	N	С	R
Benzine	0.69	1.127	1.204	С	R	R	С	R	N	N	R	R
Carbon Disulphide	1.26	0.834	0.891	R	N	R	R	R	N	N	R	R
Castor Oil	0.97	0.950	1.015	С	R	R	С	R	N	С	С	R
Cotton Seed Oil	0.93	0.970	1.037	С	R	R	R	R	N	R	R	R
Ethylene Glycol 50/50	1.12	0.884	0.945	R	R	R	R	R	R	R	С	R
Freon II	1.46	0.774	0.828	R	R	R	R	R	N	R	R	R
Gasoline	0.70	1.119	1.195	R	R	R	R	R	N	С	R	R
Glycerin	1.26	0.834	0.891	R	R	R	R	R	R	R	С	R
Kerosene	0.82	1.033	1.104	R	R	R	R	R	N	R	R	R
Liquid Propane (LPG)	0.51	1.310	1.400	R	R	R	R	R	N	N	R	R
Mineral Oil	0.92	0.976	1.042	R	N	R	R	R	N	R	R	R
Naptha	0.76	1.074	1.147	R	N	R	R	R	N	С	R	R
Perchloroethylene	1.62	0.735	0.786	С	N	R	R	R	N	N	N	R
Petroleum Oil	0.876	1.000	1.068	R	R	R	R	R	N	R	R	R
Phosphate Ester	1.18	0.862	0.921	R	R	R	R	N	R	N	R	R
Phosphate Ester Base	1.26	0.833	0.891	R	R	R	R	N	R	N	R	R
Phosphoric Acid (Acid Free)	1.78	0.701	0.749	N	N	R	N	R	N	R	N	R
Sea Water	1.03	0.922	0.985	N	N	С	С	N	R	R	R	R
Synthetic Petroleum Base	1.00	0.936	1.000	R	С	R	R	R	Ν	R	R	R
Water	1.00	0.936	1.000	N	R	R	R	N	R	R	R	R
Water Glycol 50/50	1.07	0.905	0.967	R	R	R	R	R	N	R	R	R

#### Pressure vs. Temperature Chart

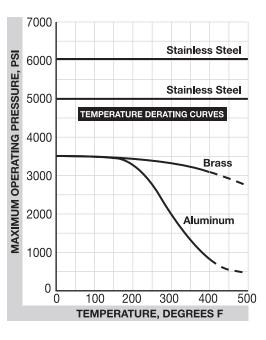


CONTINUOUS TEMPERATUREINTERMITTENT TEMPERATURE


Page 12 Form #HLIT 205-2G 11/10



# Flow vs. Pressure Drop \* Petroleum Fluids

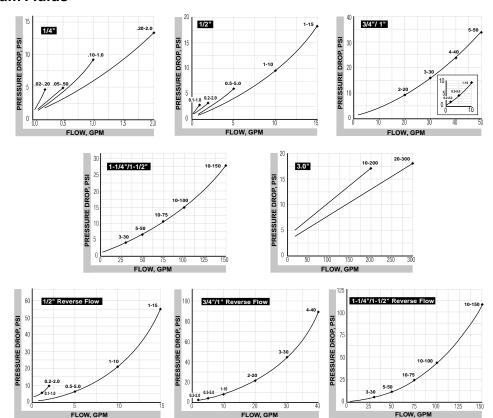

#### **Petroleum Test Kits**

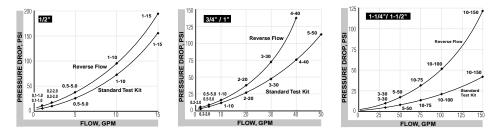



1. The pressure drop curves are valid for fluids with density and viscosity similar to factory test fluids. Fluids, especially with higher viscosity than these test fluids, will yield a higher pressure drop through the flow meter and piping system per a given flow volume.


2. A system must have adequate fluidic horsepower available to move the system fluid at a prescribed rate at a pressure adequate to overcome all pressure reducing devices – including the flow meter.





#### **Phosphate Ester**




















#### **Phosphate Ester Test Kits**










Page 14 Form #HLIT 205-2G 11/10




#### A.P.I. Oil













#### **Water-based Fluids**

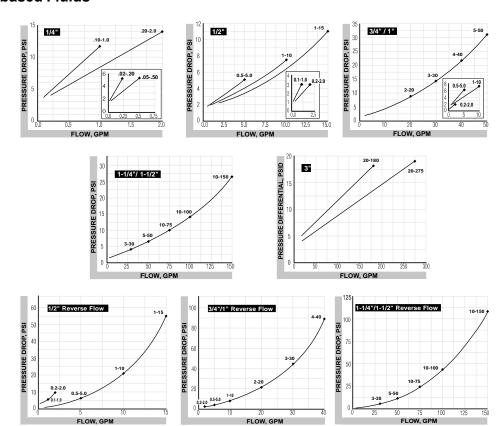


#### **Water-based Test Kits**

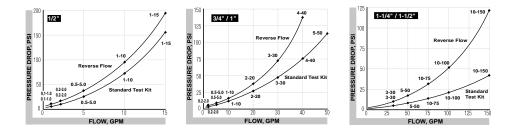


Page 16 Form #HLIT 205-2G 11/10



#### Water

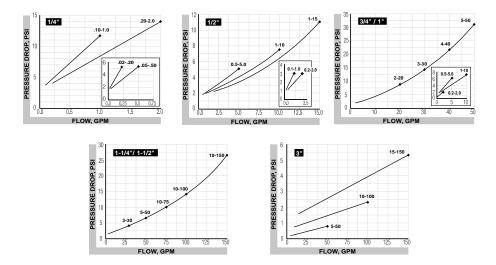

#### **Caustic and Corrosive Liquids**

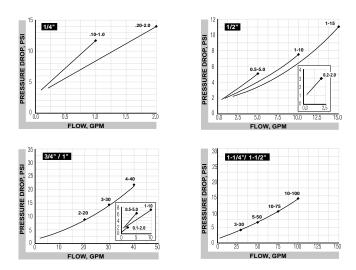





#### **Dimensions**

#### **Standard Meter**


A Nominal Port Size	B Length in (mm)	C Width in (mm)	D Depth in (mm)	E Offset in (mm)	F Flats in (mm)
1/4 (SAE 6)	4.80 (122)	1.68 (43)	1.90 (48)	.82 (21)	.88 (22)
½ (SAE 10)	6.60 (168)	2.07 (53)	2.40 (61)	1.04 (26)	1.25 (32)
3/4 (SAE 12)	7.20 (183)	2.48 (63)	2.85 (72)	1.24 (32)	1.50 (38)
1 (SAE 16)	7.20 (183)	2.48 (63)	2.85 (72)	1.24 (32)	1.75 (44)
1-¼ (SAE 20)	12.20 (310)	4.12 (105)	4.72 (120)	2.06 (52)	2.75 (70)
1-1/2 (SAE 24)	12.20 (310)	4.12 (105)	4.72 (120)	2.06 (52)	2.75 (70)






# 1-1/2 inch; C62 Flange Inches (mm)

5/8-11 UN-2B

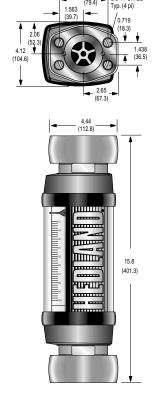


#### 3 inch; SAE, NPTF, BSPP Inches (mm)

4.50

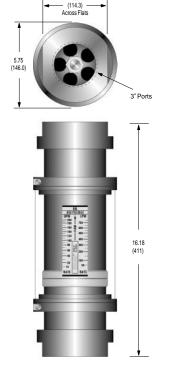

# 3 inch; C61 Flange Inches (mm)

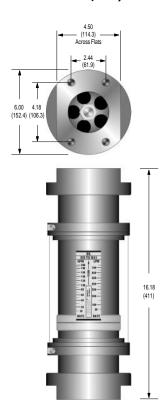

Page 18 Form #HLIT 205-2G 11/10




#### **Dimensions** (continued)

#### **High Temp Meter**

Α	В	С	D
Nominal Port Size	Length in (mm)	Width in (mm)	Flats in (mm)
1/4 (SAE 6)	6.60 (168)	2.01 (53)	1.25 (32)
½ (SAE 10)	6.60 (168)	2.01 (53)	1.25 (32)
3/4 (SAE 12)	7.20 (183)	2.48 (63)	1.50 (38)
1 (SAE 16)	7.20 (183)	2.48 (63)	1.75 (44)
1-¼ (SAE 20)	12.20 (310)	4.20 (105)	2.75 (70)
1-1/2 (SAE 24)	12.20 (310)	4.20 (105)	2.75 (70)








#### **Test Kit**

A Nominal Port Size	B Length in (mm)	B1 Length in (mm)	C Width in (mm)	D Depth in (mm)	E Offset in (mm)	F Flats in (mm)
½ (SAE 10)	6.60 (168)	9.60 (245)	2.07 (53)	2.40 (61)	1.04 (26)	1.25 (32)
¾ (SAE 12)	7.20 (183)	10.70 (272)	2.48 (63)	2.85 (72)	1.24 (32)	1.50 (38)
1 (SAE 16)	7.20 (183)	10.70 (272)	2.48 (63)	2.85 (72)	1.24 (32)	1.75 (44)
1-¼ (SAE 20)	12.20 (310)	20.50 (521)	4.12 (105)	4.72 (120)	2.06 (52)	2.75 (70)
1-1/2 (SAE 24)	12.20 (310)	20.50 (521)	4.12 (105)	4.72 (120)	2.06 (52)	2.78 (70)



#### **Return Goods Authorization**

When returning equipment for service, a Returned Goods Authorization (RGA) number must be obtained from our Service Department. Please contact them by phone at 800-433-5263 or 262-639-6770 or by e-mail to hedlandsales@racinefed.com.

All returns go to the following address and must include the RGA number on the outside of the box:

Hedland
Division of Racine Federated Inc.
8635 Washington Avenue
Racine, WI 53406-3738 USA

Attn: RGA # xxx-xxxx



#### LIMITED WARRANTY and DISCLAIMER

Hedland, Division of Racine Federated Inc. warrants to the end purchaser, for a period of one year from the date of shipment from the factory, that all flow meters manufactured by it are free from defects in materials and workmanship. This warranty does not cover products that have been damaged due to misapplication, abuse, lack of maintenance, or improper installation. Hedland's obligation under this warranty is limited to the repair or replacement of a defective product, at no charge to the end purchaser, if the product is inspected by Hedland and found to be defective. Repair or replacement is at Hedland's discretion. A returned goods authorization (RGA) number must be obtained from Hedland before any product may be returned for warranty repair or replacement. The product must be thoroughly cleaned and any process chemicals removed before it will be accepted for return.

The purchaser must determine the applicability of the product for its desired use and assumes all risks in connection therewith. Hedland assumes no responsibility or liability for any omissions or errors in connection with the use of its products. Hedland will under no circumstances be liable for any incidental, consequential, contingent or special damages or loss to any person or property arising out of the failure of any product, component or accessory.

All expressed or implied warranties, including the implied warranty of merchantability and the implied warranty of fitness for a particular purpose or application are expressly disclaimed and shall not apply to any products sold or services rendered by Hedland.

The above warranty supersedes and is in lieu of all other warranties, either expressed or implied and all other obligations or liabilities. No agent or representative has any authority to alter the terms of this warranty in any way.





Materials & specifications are subject to change without notice.

HEDLAND is a registered trademark of Racine Federated Inc.
VITON is a registered trademark of DuPont Dow Elastomers.
CELCON is a registered trademark of Hoeschst Celanese Corporation.
PYREX is a registered trademark of Corning Glass Works Corporation.
TEFLON is a registered trademark of E.I. du Pont de Nemours and Company.
UL is a registered trademark of Underwriters Laboratories.





**DYNASONICS** Flo-t





