


Medical Grade Silicone Tubing & Extrusions

USP Class VI Biocompatible Materials



With in-house tooling capabilities, Parker's Medical Systems Division offers biomedical and pharmaceutical OEMs a wide range of medical grade single and multi-lumen tubing as well as extruded profiles. Along with x-ray striped and x-ray opaque extrusions, Parker's Medical Systems Division specializes in medical grade wire-reinforced, non-occluding silicone tubing that are used to manufacture adult and pediatric catheters.

All of Parker's Medical Systems Division's tubing and extruded profiles are manufactured in an FDA Registered, ISO 13485 facility and are continuously monitored on the line for dimensional tolerances.

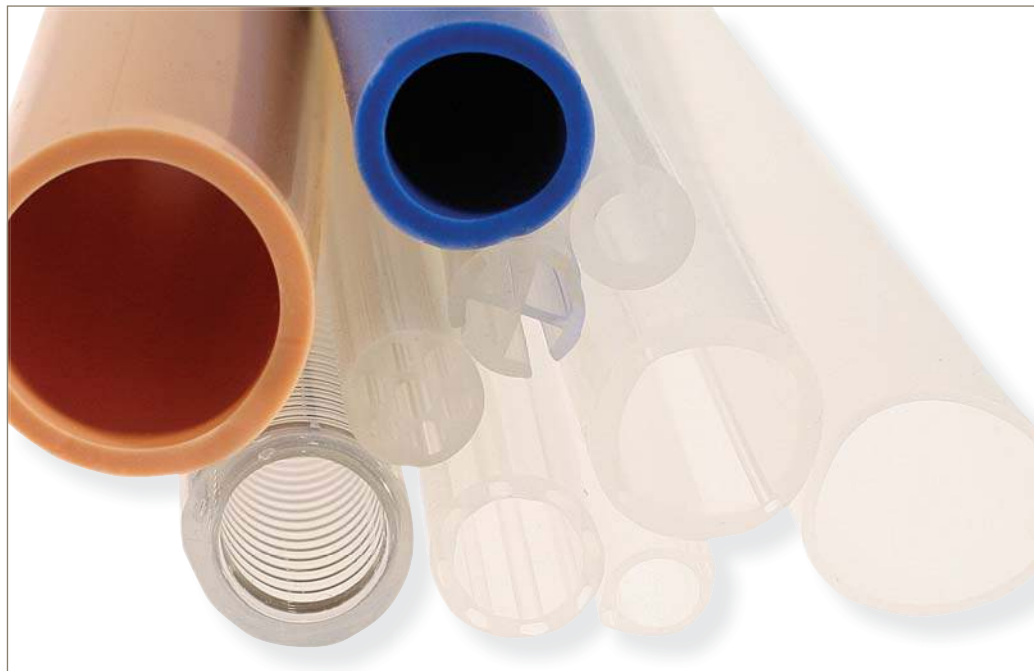

Contact Information:

Parker Hannifin Corporation
Medical Systems Division
3191 E. La Palma Avenue
Anaheim, CA 92806 USA

phone 714 632 7710
fax 714 632 5647
Techsales@parker.com

www.parker.com

Product Benefits:

- All extrusions are platinum-cured.
- All extrusions do not contain any peroxides.
- All extrusions are manufactured with silicone materials from Dow Corning, Momentive, NuSil, Shin-Etsu, and Wacker that will pass ISO 10993 tests.
- All extrusions are manufactured in ISO Class 8 Cleanrooms.
- All extrusions can be sterilized with autoclave, ethylene oxide, or gamma radiation.



ENGINEERING YOUR SUCCESS.

Tubing Sizes:

Parker’s Medical Systems Division’s tubing and extruded profiles are manufactured to biomedical and pharmaceutical OEMs’ dimensional specifications. Most commonly used medical grade tubing sizes, along with their tolerances are listed in the tubing chart shown.

Tubing is packaged in 50 foot coils (15.24 meters), double bagged and shipped in crush-resistant boxes. Material certification and lot traceability are included in every box.

Custom sized tubing with ID’s ranging from 0.012” to 1.0” with desired wall thickness can be extruded and cut to length per our customers’ exact written specifications.

Recommended for use in:

- Peristaltic pumps
- Multi-lumen catheter mainshafts
- Wound drainage tubes
- Enteral feeding catheters
- Spring reinforced catheters
- Peritoneal dialysis catheters
- Tracheostomy tubes
- Foley catheter mainshaft and cuffs
- Vascular loops

| INSIDE DIAMETER | | OUTSIDE DIAMETER | | WALL | |
|-----------------|-------|------------------|-------|------|------|
| Inch | mm | inch | mm | inch | mm |
| .012 | .31 | .025 | .64 | .006 | .15 |
| .020 | .51 | .037 | .94 | .008 | .20 |
| .025 | .64 | .047 | 1.19 | .011 | .28 |
| .030 | .76 | .065 | 1.65 | .018 | .46 |
| .040 | 1.02 | .085 | 2.16 | .023 | .58 |
| .058 | 1.47 | .077 | 1.96 | .009 | .23 |
| .062 | 1.58 | .095 | 2.41 | .016 | .41 |
| .062 | 1.58 | .125 | 3.18 | .032 | .81 |
| .078 | 1.98 | .125 | 3.18 | .024 | .61 |
| .104 | 2.64 | .192 | 4.88 | .044 | 1.12 |
| .132 | 3.35 | .183 | 4.65 | .026 | .66 |
| .125 | 3.18 | .250 | 6.35 | .063 | 1.59 |
| .188 | 4.76 | .313 | 7.94 | .063 | 1.59 |
| .188 | 4.76 | .375 | 9.53 | .094 | 2.38 |
| .250 | 6.35 | .375 | 9.53 | .063 | 1.59 |
| .250 | 6.35 | .438 | 11.11 | .094 | 2.38 |
| .250 | 6.35 | .500 | 12.70 | .125 | 3.18 |
| .313 | 7.94 | .500 | 12.70 | .094 | 2.38 |
| .375 | 9.53 | .500 | 12.70 | .063 | 1.59 |
| .375 | 9.53 | .563 | 14.29 | .094 | 2.38 |
| .375 | 9.53 | .625 | 15.88 | .125 | 3.18 |
| .500 | 12.70 | .688 | 17.46 | .094 | 2.38 |
| .500 | 12.70 | .750 | 19.05 | .125 | 3.18 |
| .625 | 15.88 | .875 | 22.23 | .125 | 3.18 |
| .625 | 15.88 | .938 | 23.82 | .156 | 3.97 |
| .750 | 19.05 | 1.000 | 25.40 | .125 | 3.18 |



This document and other information from Parker Hannifin Corporation, its subsidiaries and authorized distributors provide product or system options for further investigation by users having technical expertise.

- The user, through its own analysis and testing, is solely responsible for making the final selection of the system and components and assuring that all performance, endurance, maintenance, safety and warning requirements of the application are met. The user must analyze all aspects of the application, follow applicable industry standards, and follow the information concerning the product in the current product catalog and in any other materials provided from Parker or its subsidiaries or authorized distributors.

- To the extent that Parker or its subsidiaries or authorized distributors provide component or system options based upon data or specifications provided by the user, the user is responsible for determining that such data and specifications are suitable and sufficient for all applications and reasonably foreseeable uses of the components or systems.

